



AN1006 – Hologic Combination Measurement

- Make sure all hardware is connected and the system is in the "Ready" state.
- Select W/AI from the drop-down list located on the bottom right.

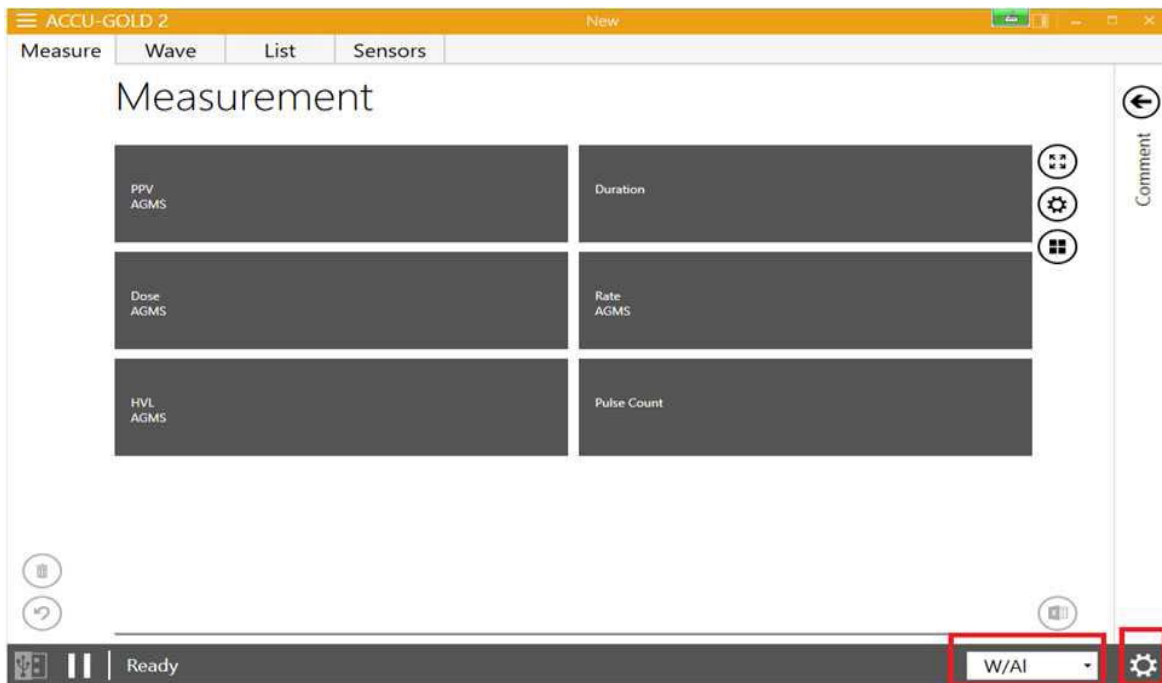


- Click on the Settings button on the bottom right and set "End of Exposure Delay" to 3 seconds. If additional time is required change to 5 seconds.

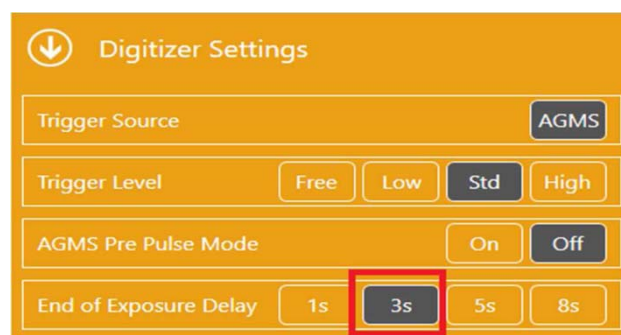


AN1006 – Hologic Combination Measurement

- Run the measurement

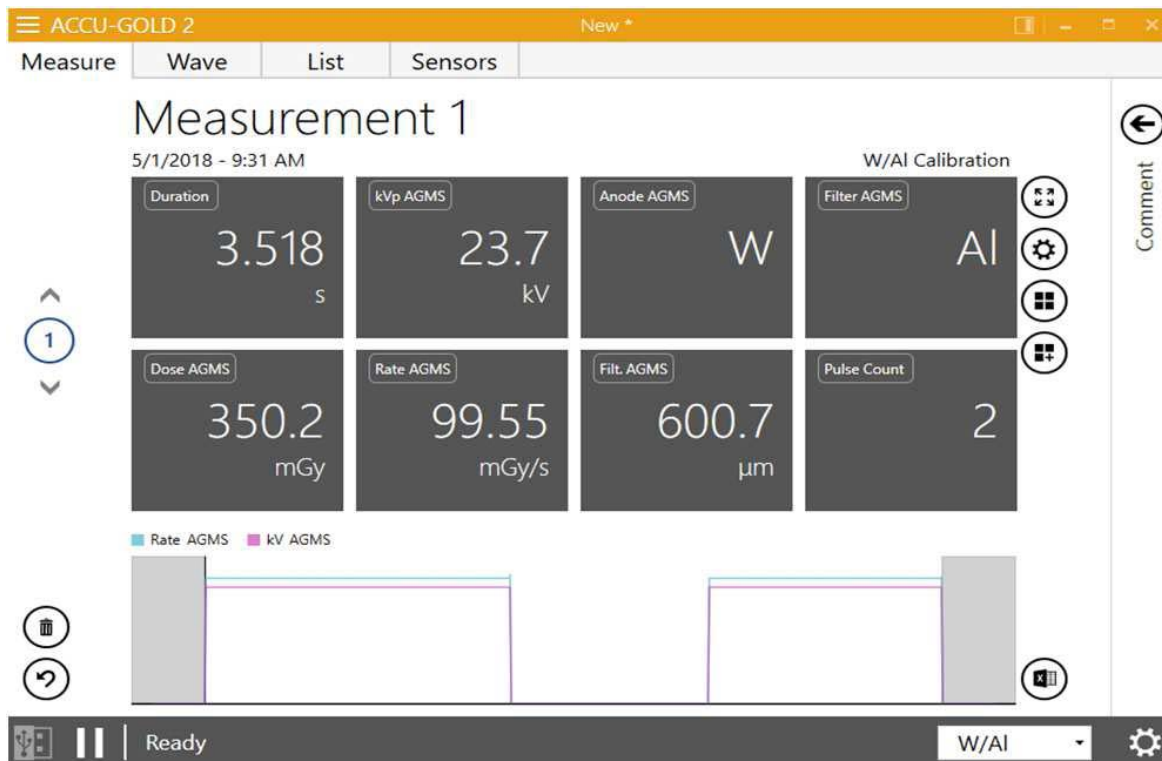


- Click on the "Wave" tab on the upper left and left-click the beginning and end of the W/AI section to lock the region of interest.

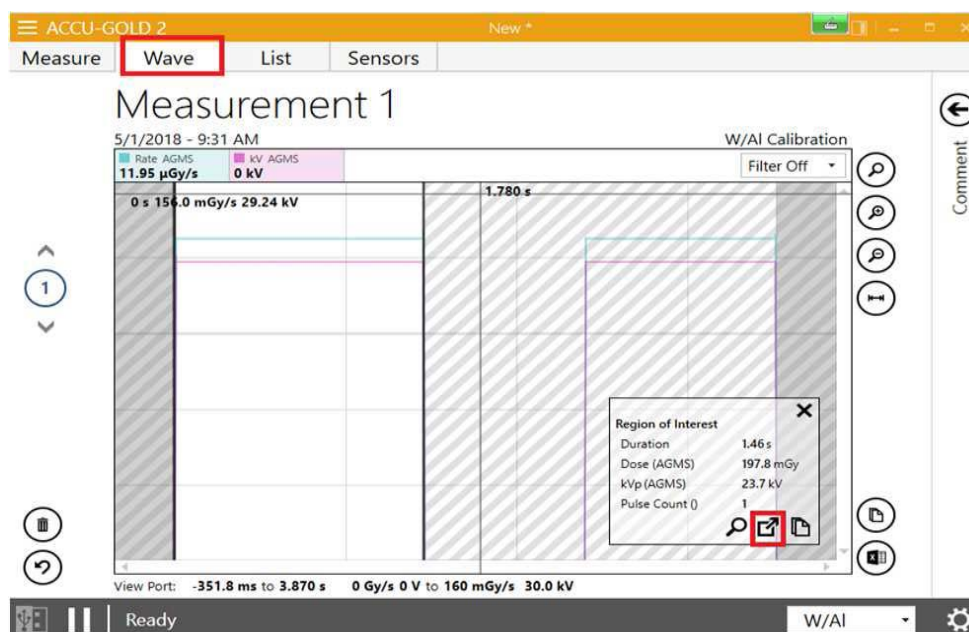


AN1006 – Hologic Combination Measurement

- Click the "Extract" button to create a daughter measurement using only the selected data.

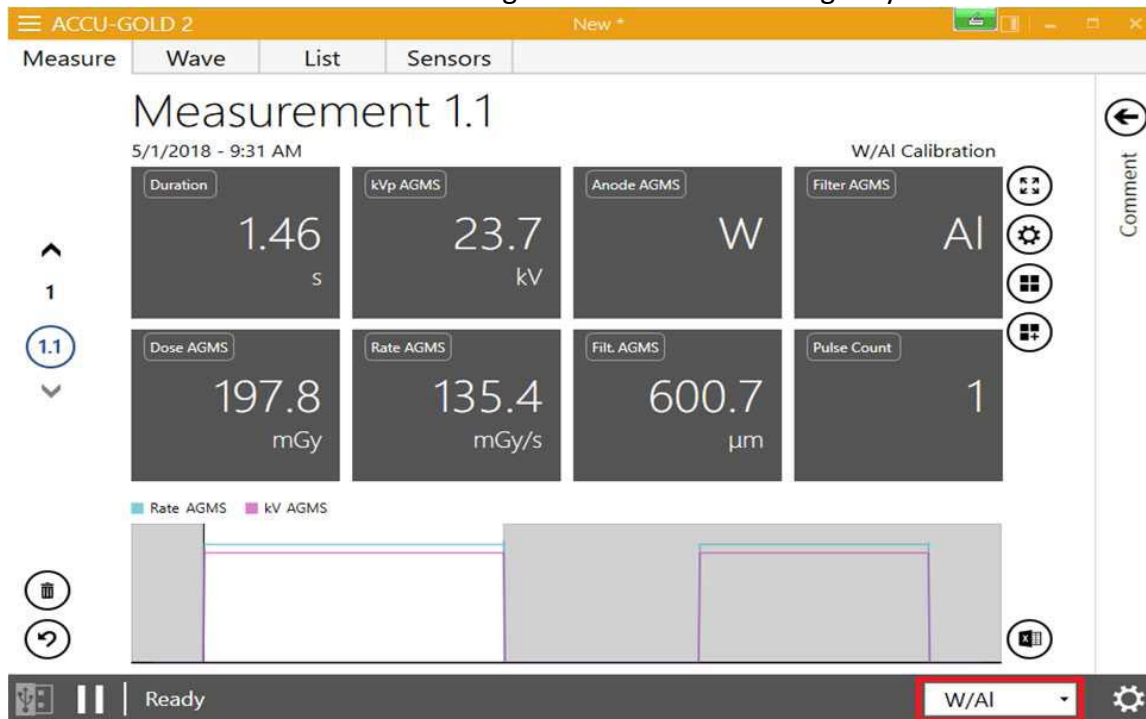


- You can now switch the anode filter to W/Rh and repeat the same exposure

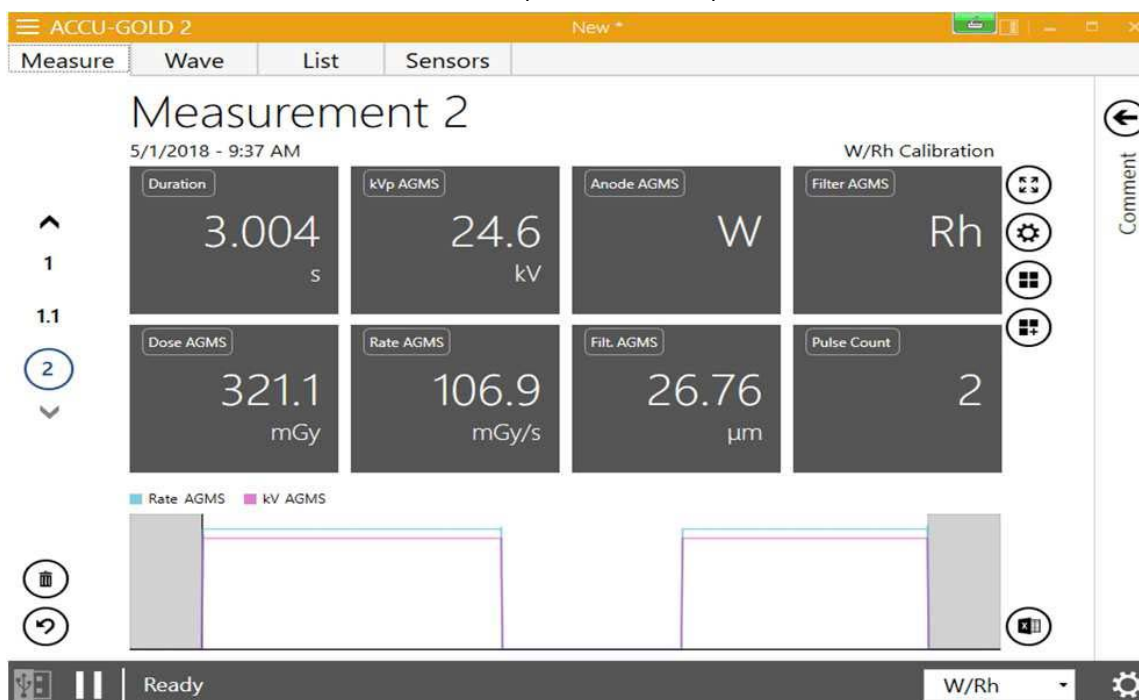

AN1006 – Hologic Combination Measurement

- Select the W/Rh region of interest and extract to a daughter measurement

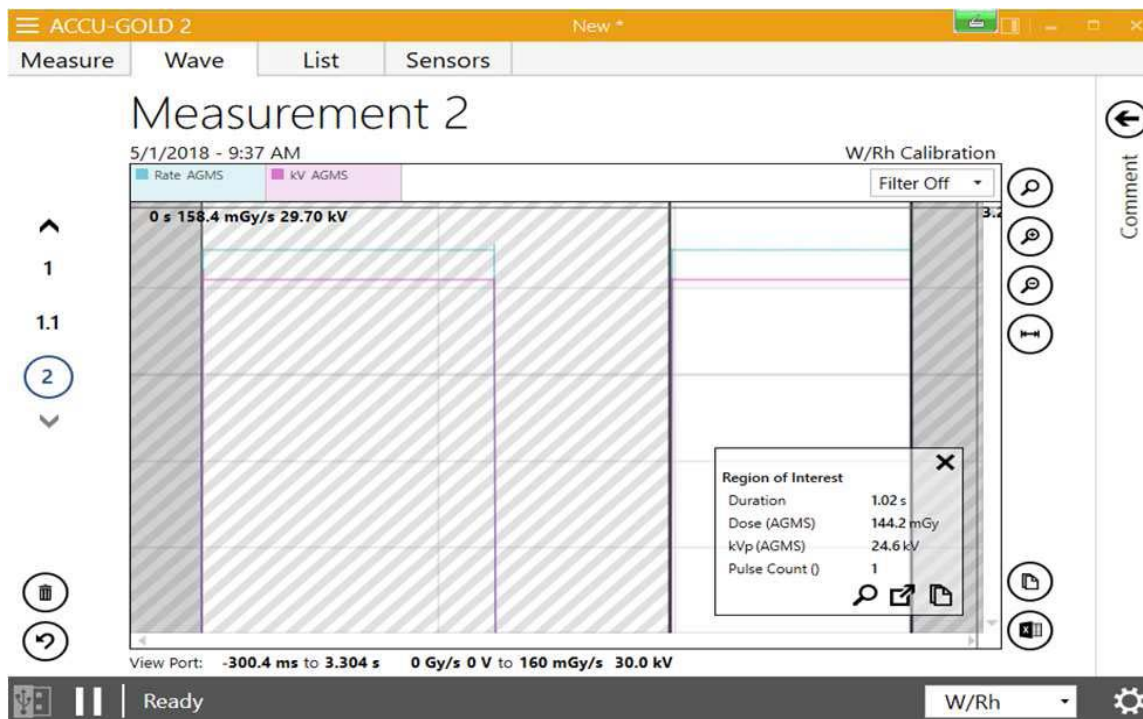

- You can now tally the Dose from the W/AI and W/Rh daughter measurements for a total.

