

Accu-Gold Nugget Wi-Fi Module

(For use with Accu-Gold Digitizers)



Radcal

Radcal
426 West Duarte Road
Monrovia, CA 91016-4591 USA
USA (626) 357-7921
Fax USA (626) 357-8863
email sales@radcal.com
www.radcal.com

Radcal Part # MNL/AGNUGGET
4094277 Rev:C2
Printed: Apr, 2024

Introduction

Thank you for choosing the AGNUGGET, the Accu-Gold Wi-Fi Module.

For more in-depth information or troubleshooting, contact Customer Support at (626) 357-7921 x 123 or email Cust_Sup@Radcal.com

Overview

The Accu-Gold Nugget provides a wireless connection between the Accu-Gold measurement system and the display device or computer. It contains a micro computer that relays information via Wi-Fi to the desktop or tablet running the Accu-Gold software. It uses a built-in Lithium-ion polymer battery with battery management circuitry that maintains the life of the battery by carefully controlling the charging while monitoring its temperature and voltage.

Package contents


	<u>Radcal Part Number</u>
Accu-Gold Nugget	MDL/AGNUGGET
Charger (5V, 1.8A) PRS/PSAC09R-050	PRS/PSA10F-050
AC power supply blades (US) or	(built in)
AC power supply blades (international kit)	PRS/PSA10F-Q(D)
Flash drive with the latest Accu-Gold software	MDL/AG2SW
<i>Flash Drive adapter, USB A female to mini USB B female</i>	<i>CBL/USB-AF2MBF</i>

System Requirements

Operating system - Windows 7, 8, 10
(Windows XP not supported)

Accu-Gold V2 or greater software required
(Version 1 is not supported).

(Note: Accu-Gold Excel and Accu-Gold Excel Templates are not supported)

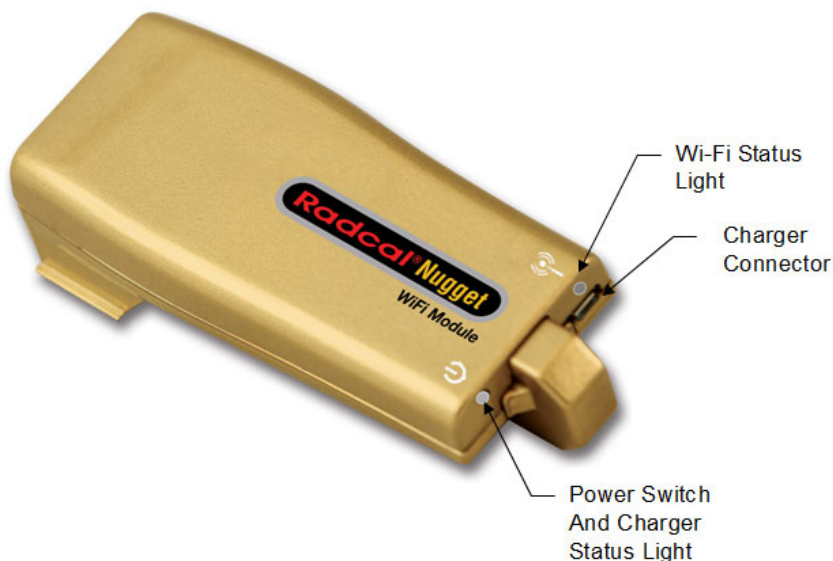

Power Switch Status

Solid Green
Blinking Green
Blinking Yellow
Solid Yellow
Long on-off pause (4 sec)

Meaning

Power On
Low Battery (~25% remaining)
Battery Charging
Battery Fully Charged
Battery Error

Wi-Fi Status

Orange
Blinking Green
Red

Meaning

Starting
Wi-Fi Ready
Error

Additional indications:

Fast blinking orange is used to indicate firmware update has been completed.

Operation

This manual does not cover software and device driver installation. For information on installing the software and driver, see the readme file located on the flash drive included with your Accu-Gold device.

Install Accu-Gold software version 2.

Snap the Nugget onto the digitizer module:



Align the USB connectors and slide the Nugget all the way in. (To remove it, pull out the connector first then unsnap it by tilting it upward or sliding it off the end of the digitizer.)

Plug in a multi-sensor, ion chamber or dose diode.

Press the power button on the Nugget. The power button will turn green. (If the charger is plugged in, it will blink yellow.) The Wi-Fi status light will turn on displaying green and then orange. When it blinks green, it is ready to connect.

Start the Accu-Gold 2 software.

Click on **Connect via Wi-Fi**. The software will detect the presence of the Nugget and connect to it automatically.

You are now ready to start.




Connecting manually

If the Nugget is not able to connect automatically, you will need to connect manually. If there are multiple Nuggets that show up, you will also have to connect manually.




For Windows 10, if you get this dialog box, click on "Connect using a security key instead"

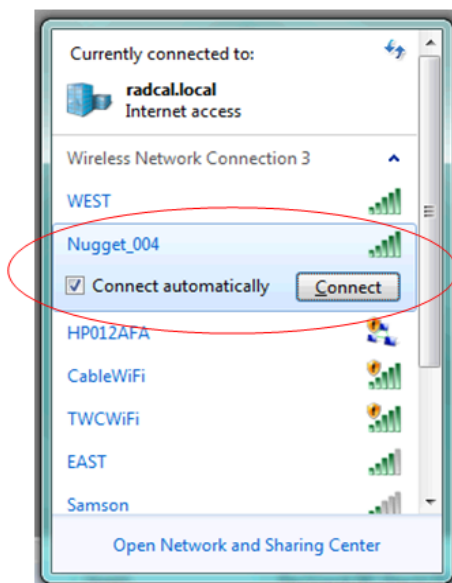

On the computer, check the Wireless Network Connection pane.

There, you will find "Nugget_51-xxxx" as one of the Wi-Fi devices (the ID number will be the Nugget_serial number). Click on the Nugget and when asked for the **password**, enter **12345678**.

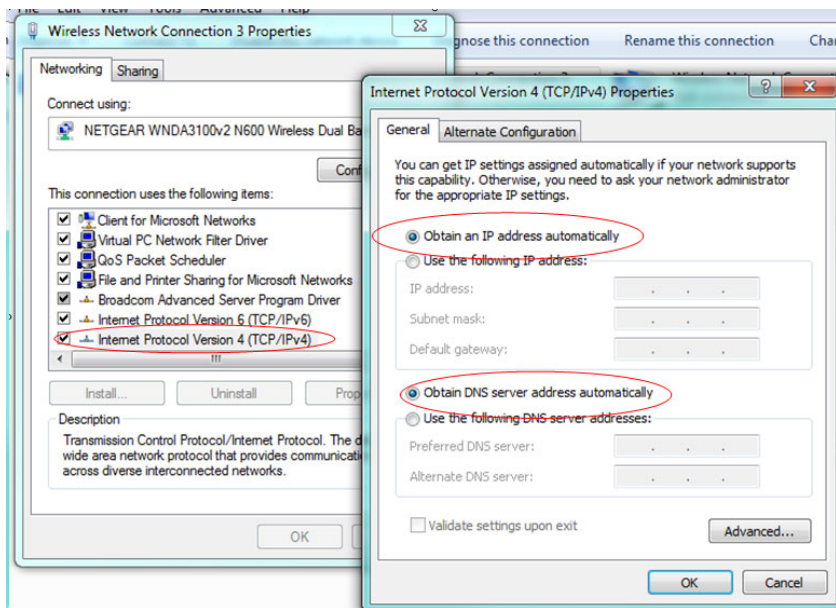

NOTE: Internet Protocol Version 4 (IPv4) must not be set to a fixed IP address. IPv4 must be set to “Obtain an IP address automatically” and “Obtain DNS server address automatically. Contact us if any issues arise.

Start the Accu-Gold 2 software.

Click on “Connect via Wi-Fi”.
You are now ready to start.

Note that not all sensors, measurements and modes of the Accu-Gold software are available when using the Nugget. See Appendix A for a comparison list.

Battery

3.7V Li-ion polymer 1150mAh single cell - not removable.

Battery life will depend on how it is being used. Turn off the unit when it is not being used to conserve battery life. Turning the unit back on will require the unit to re-establish the Wi-Fi connection which may take a minute or so at most. The Nugget will turn itself off to conserve battery life.

Power Saving features

The Nugget will go into sleep mode as much as possible. After a longer idle time, the Nugget will go into a lower power mode. After 10 minutes, if left unattended, the Nugget will power off.

Battery Charger

The battery management circuitry prevents over-charging and over-usage. When the battery level drops to approximately 25%, the power LED will start to blink green.

The charger that is supplied with the Nugget has been chosen to optimize the charging of the battery. The power-status light shows yellow when the charger is plugged in. Blinking yellow means that it is charging, solid yellow means that the charging is complete. The Nugget can be used while being charged and the charger may be left connected indefinitely. Typical charging time for a fully drained battery is approximately 3 hours.

If the battery has been exhausted, there will be a small delay while it charges up enough to operate.

The Nugget can be charged using other chargers or even using the USB port of a computer but the charging time may vary depending on the source and how it is recognized.

Note: firmware updates will be provided from time to time. In order to install an update, the charger supplied with the Nugget **WILL** be required.

Physical description

Dimensions	135 mm x 62 mm x 33 mm (5.3" x 2.4" x 1.3")
Weight	0.12 kg (0.25 lbs)

Environmental Conditions

Operating temperature:

15 °C to 35 °C

Pressure:

60 to 105 kPa

Humidity:

Up to 80% RH or 20 g/m³

Storage Temperature:

-20 °C to +60 °C

Wi-Fi specs

Network Standard Support: IEEE 802.11b/g/n

Frequency band: 2.400 - 2.472 Ghz, channels 1-11

Antenna power: <10 mW/MHz

Connectivity: Access Point mode

Wireless Security: WPA2

Networking protocol: TCP

NOTE:

This equipment shares a frequency band with a wide range of equipment: e.g. industrial, scientific, and medical equipment such as microwave ovens, premises radio stations (radio stations requiring licenses), and specified low-power radio stations (radio stations not requiring licenses), for RFID used for factory production lines as well as amateur radio stations (radio stations requiring licenses).

1. Before use, confirm that no premises radio stations and specified low-power radio stations for RFID or amateur radio stations operate in your vicinity.
2. In the event that this equipment causes harmful interference to any premises radio station for RFID, immediately halt radio wave emission and contact Customer Support for consultation on interference avoidance measures (e.g. partition installation).
3. Contact Customer Support if this equipment causes harmful interference to any specified low-power radio stations for RFID or amateur radio stations or if other problems arise.

Appendix A

Measurement Feature Comparison

Document Version 4 (2015-08-03)

Using Accu-Gold V2 software

<u>Feature</u>	<u>USB</u>	<u>Nugget</u>
Support for AGDM	yes	yes
Support for AGDM+	yes	yes
10 kHz Signal Sampling	yes	yes
Support for AGMS-D Sensor	yes	yes
Support for AGMS-M Sensor	yes	yes
Support for AGMS-DM+ Sensor	yes	yes
Support for AGMS-D+ Sensor	yes	yes
Support for AGMS-M+ Sensor	yes	yes
Support for Ion Chambers	yes	yes
Support for Dose Diodes	yes	yes
Support for Light Sensor	yes	yes
Support for Current Clamp	yes	yes
Support for Current Sensor	yes	yes
Setting for End of Exposure Delay	yes	yes
Setting for Trigger Level	yes	yes
Setting for AGMS Calibration	yes	yes
Setting for IC Wave Mode	yes	yes
AGMS Corrections for Dose, HVL and kV	yes	yes
Ion Chamber Stabilization	yes	yes
Max Exposure Length	300 sec	40 sec
PrePulse Detection Mode	yes	yes
FreeRun Mode	yes	yes
TimeStamp for Measurement	yes	yes
Dose, Dose Rate, Time Results for AGMS, IC and DD	yes	yes
AGMS Ave kV, HVL, Filtration	yes	yes
Error Handling and Messages	yes	yes
Records all Sensor Serials	yes	yes
Support for Wave Bandwidth Filtering	yes	yes
Support for Region of Interest	yes	yes

Handling of legacy IC chambers	yes	yes
AGMS kVp Result	yes	yes
AGMS PPV Result	yes	yes
Max Sensor Rate Results	yes	yes
Min Sensor Rate Results	yes	not planned
Duty Cycle Results	yes	yes
Pulse Frequency	yes	yes
Ave Pulse Width Result	yes	yes
Max Pulse Width Result	yes	not planned
Min Pulse Width Result	yes	not planned
Dose / Pulse Result	yes	yes
Pulse Count	yes	yes
IC Temperature Result	yes	yes
IC Air Pressure Result	yes	yes
Reads temp and pressure on start	yes	yes
Updates calibrations, temp and pressure for each measurement	future	yes
Dose Ratios Results	yes	yes
Report dose without kV	yes	yes

Sensor availability comparison	AG V2 with USB	AG V2 with Nugget
AGMS multisensor	yes	yes
AGMS+ multisensor	yes	yes
Ion Chamber	yes	yes
Dose Diode	yes	yes
mAs sensor	yes	yes
Light Sensor	yes	yes

Appendix B

Firmware update

Turn off the Nugget.

NOTE: If the battery is exhausted, charge it for at least ten minutes before attempting a firmware update.

Required Equipment: **DO NOT SUBSTITUTE!**

PRS/PSAC09R-050 CHARGER, 5VDC, 1.8A USB MICRO

CBL/USB-AF2MBF ADAPTER, USB A FEM TO MINI B FEM

Flash drive with new Nugget firmware

Assemble as shown:



Flip it over and observe the WiFi light.



Press the power-on button of the Nugget. The Wi-Fi light will come on GRN then ORN. When it starts blinking orange quickly, the update is complete. Unplug the flash drive, press the Nugget power button to turn it off and then back on again. It is now ready to use.

Appendix C

Warranties and Disclosures

Warranty for the Accu-Gold Measurement System

Radcal Corporation warrants that, in the event that any defects in material or workmanship should develop within one year of the date of shipment, the company assumes full responsibility for servicing equipment of its manufacture without charge upon return of the equipment to Radcal, with shipping costs prepaid by the customer. Costs to return-ship to customer by ground transportation will be paid by Radcal if the repairs are warranty-applicable. This warranty excludes batteries.

Radcal shall not be held liable for damages or delays caused by defects beyond making repairs or furnishing replacement parts, nor shall Radcal be liable for any defective material replaced without Radcal's consent during the period of this warranty. Radcal reserves the right to perform warranty services at its own factory.

Non-Warranty Repairs

The calibration of this instrument was correct within specified limits when the instrument left our factory. Radcal cannot be responsible for injury or damage resulting from improper use or calibration errors which develop subsequent to our shipment of the instrument. If Radcal determines that a fault has been caused by misuse, abnormal operating conditions, or repairs by unauthorized personnel during the warranty period, repairs and shipping costs will be billed at normal rates.

If the equipment is found to be in proper working condition, Radcal will return-ship the equipment at customer expense.

Data Loss

Although we take great effort to save your data, the customer is responsible for backing up any and all data that is stored on their computers prior to being serviced.

WEEE and RoHS

Radcal meets the requirements of the Directive 2012/19/EU on Waste Electrical and Electronic Equipment, and has implemented full compliance. Recycling manuals are available on request.

The Accu-Gold Nugget meets the requirements of the 2011/65/EU (RoHS) Directive.

Appendix D

Declaration of Conformity

According to Test Report No. 97339-4 and 97339-5

Manufacturer's Name: Radcal Corporation
Manufacturer's Address: 426 West Duarte Road
Monrovia, CA 91016
U.S.A.

Declares that the Product

Product Name: Accu-Gold Wi-Fi Module
Model Number(s): AGNUGGET
Product Accessories: All

Conforms to the following Product Specification:

EMC: EN61326-1 (2006) Group 1 Class A
EN 61000-4-2 (1995) +A1 +A2
EN 61000-4-3 (2002)
EN 61000-4-4 (2004)
EN 61000-4-6 (2009)

The product herewith complies with the RFI-emissions¹ requirements and immunity requirements and carries the CE marking accordingly.

E. MacIntosh
Engineering
10 Aug 2015

¹ This product is known to cause interference when used with the charger connected and powered. If interference occurs in a particular installation the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the instrument.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Use it without the charger.

Appendix E

Regulatory

EU (ETSI):

This device is intended for home and office use in all EU countries (and other countries following the EU directive 1999/5/EC).

FCC:

Contains FCC ID: XF6-RSWC201

This device complies with the Part 15 of the FCC Rules.

(1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

FCC RF Radiation Exposure Statement:

This equipment complies with FCC RF radiation exposure limits set forth for an uncontrolled environment. This device and its antenna must not be co-located or operating in conjunction with any other antenna or transmitter. To comply

with FCC RF exposure compliance requirements, this grant is applicable to only Mobile Configurations. The antennas used for this transmitter must be installed to provide a separation distance of at least 20 cm from all persons and must not be co-located or operating in conjunction with any other antenna or transmitter.


Industry Canada Statement:

Contains: IC: 8407A-RSWC201

This device complies with RSS-210 of the Industry Canada Rules.

Japan (Telec)

Contains: Telec Construction Certification Number
001-A13582.



The Wi-Fi module used by the Nugget has been certified for use in Japan.

(1) "2.4": Represents radio equipment using the 2.4 GHz band.

(2) "DS/OF": Represents modulation system (refer to Section 2.4.1 for details²).

(3) "4": Represents estimated interference-causing radius to premises radio stations for RFID (refer to Section 2.4.2 for details¹).

(4) "■ ■ ■": Indicates that the equipment can use the entire band and is capable of avoiding the band used by RFID systems (refer to Section 2.4.3 for details²).

China PRC (CMIIT)

The equipment contains the RF modules of which Type
Approval code is CMIIT ID: 2014DJ6439